Removing the Type II Enclosure

1. Install Shipping Locks (see CFM Manual for help).
2. Remove 1/4x20” nuts from the studs on the enclosure.
3. Carefully maneuver the enclosure off and around the measurement pan without any contact.

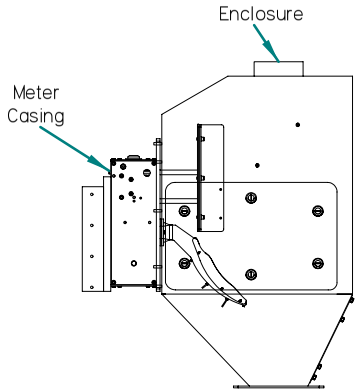

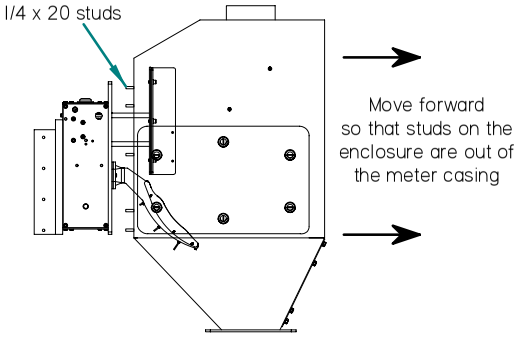

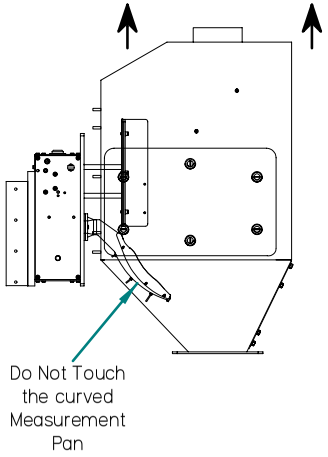

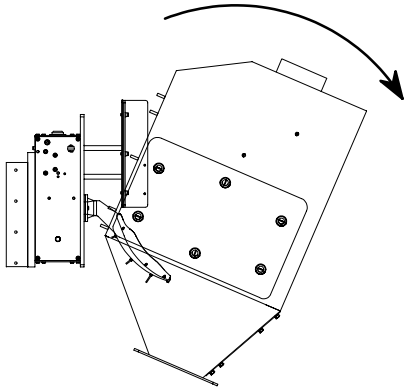

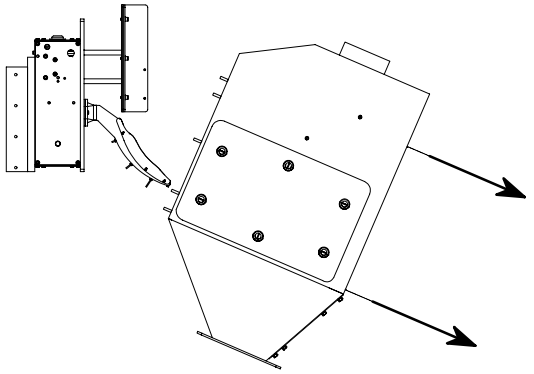

EASTERN INSTRUMENTS · 416 LANDMARK DRIVE · WILMINGTON NC 28412
phone: 910.392.2490 · fax: 910.392.2123 · website: www.easterninstruments.com